



1 discard    proceed    2 discard




Discard (hemolysed)

- 1 Keep tube in rack on ice pack and use immediately. Do not hold tube from tube barrel to avoid warming contents.
- 2 Warm tube in palm of hand for 20 seconds.

**CAUTION and TIPS:**

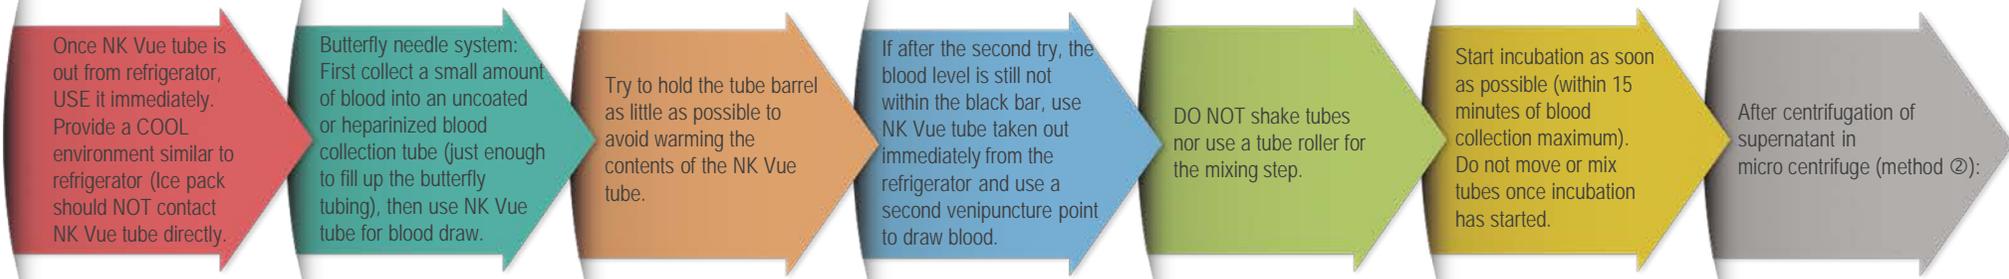

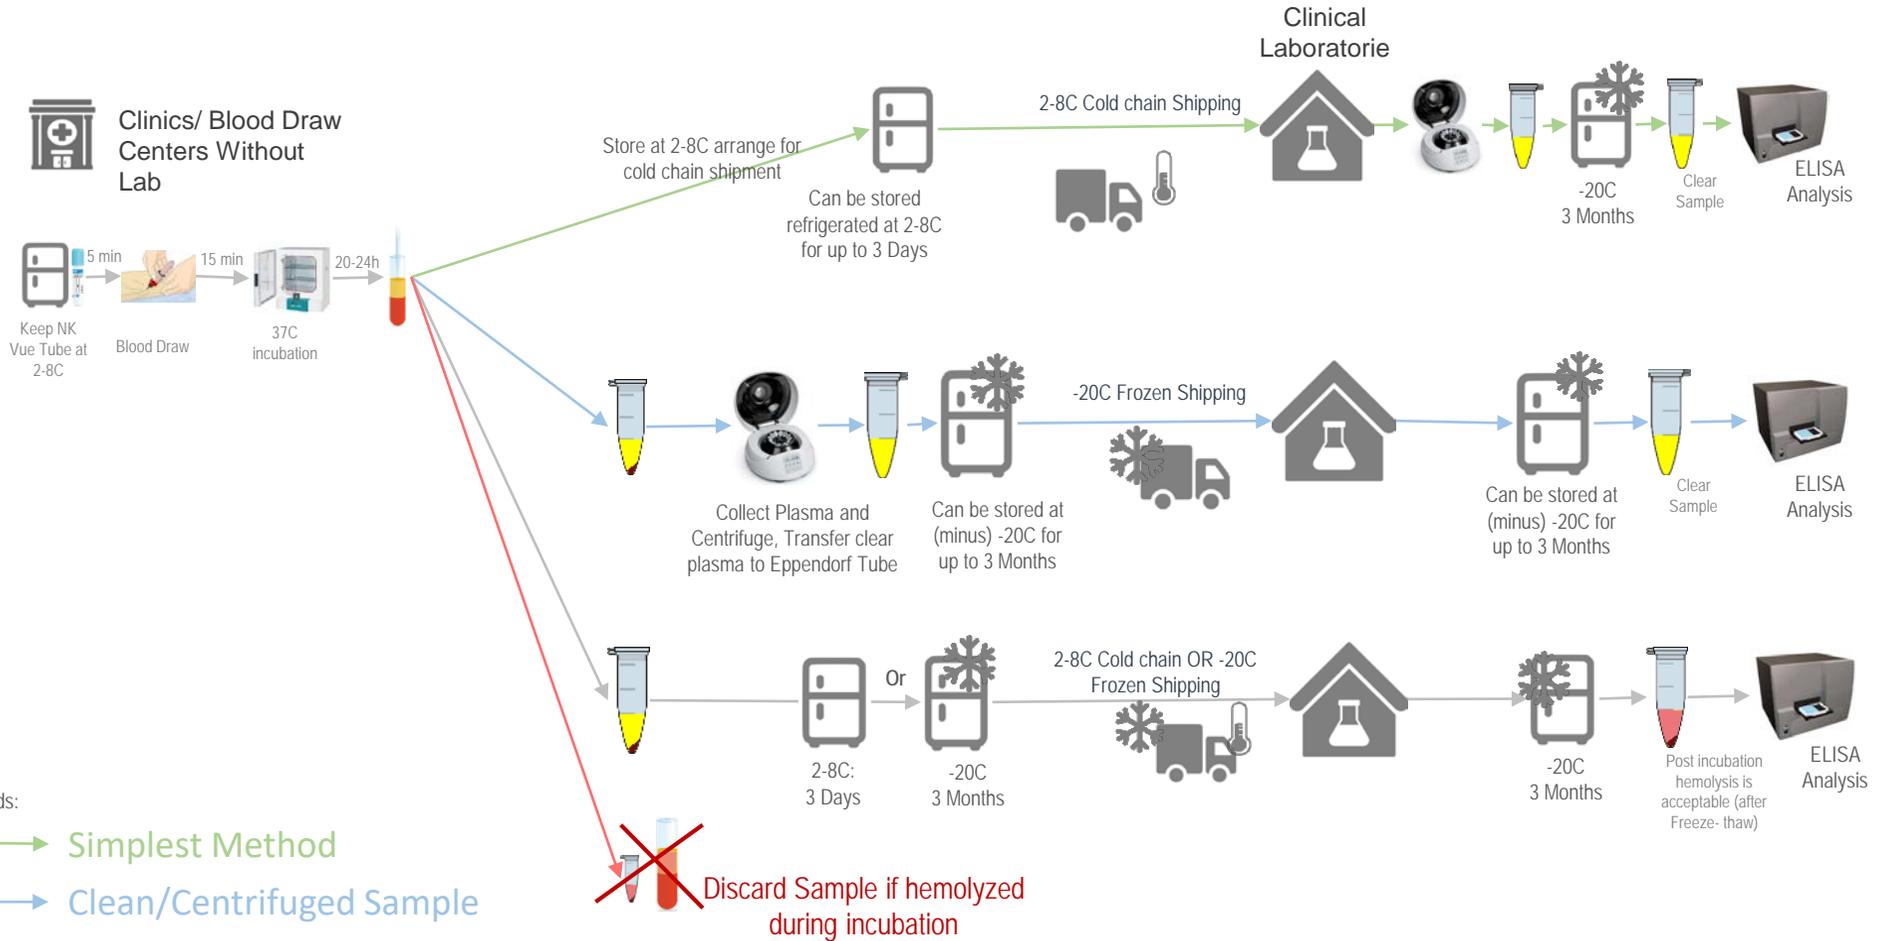

Methods:

- ① → Simplest Method
- ② → Clean/Centrifuged Sample
- ③ → Acceptable Method